



Agilent Technologies, Inc. Case 10011219-4
Inv: Richard A. Nygaard Jr. SN: 10/824680
Title: Method And Apparatus For Performing Eye
Diagram Measurements

Page 1 of 2

3/4


20 EACH PARALLEL LINE IS A MEASUREMENT REGION: (V_N CROSSED V_T DURING dt)

A RESOLUTION
RECTANGLE OF
 ΔV & ΔT

DATA CAPTURE
REFERENCE (T_g)

Δt (NO RELATION TO ΔT_{SAMP})

21

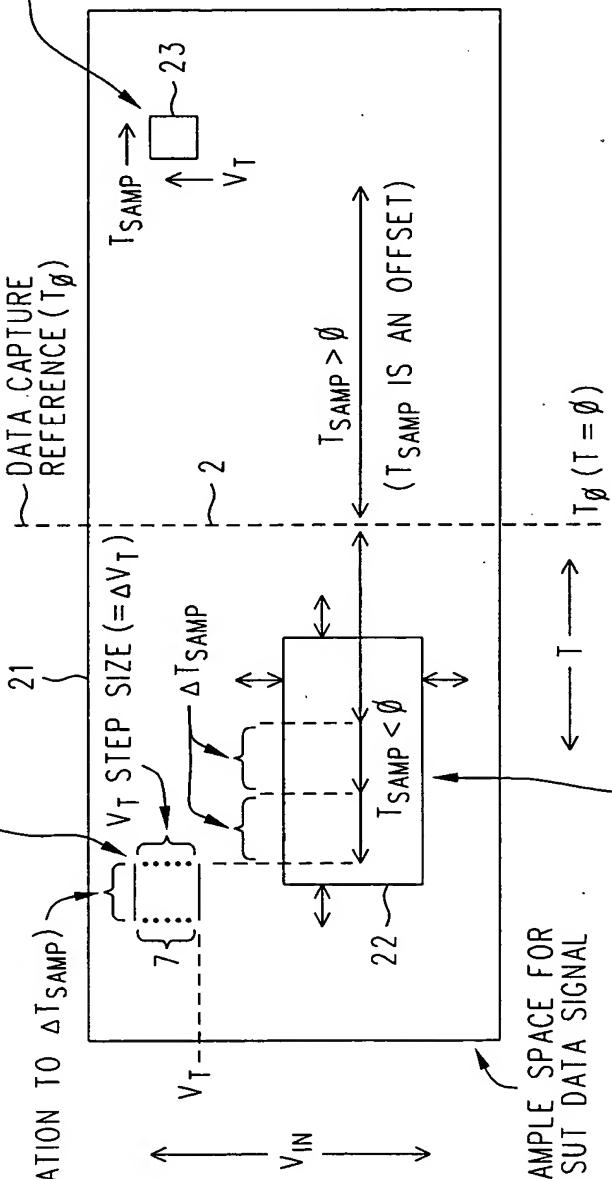

- A SELECTABLE SIZE FIELD OF VIEW
FOR DISPLAYING RENDERED EYE DIAGRAMS

FIG. 3

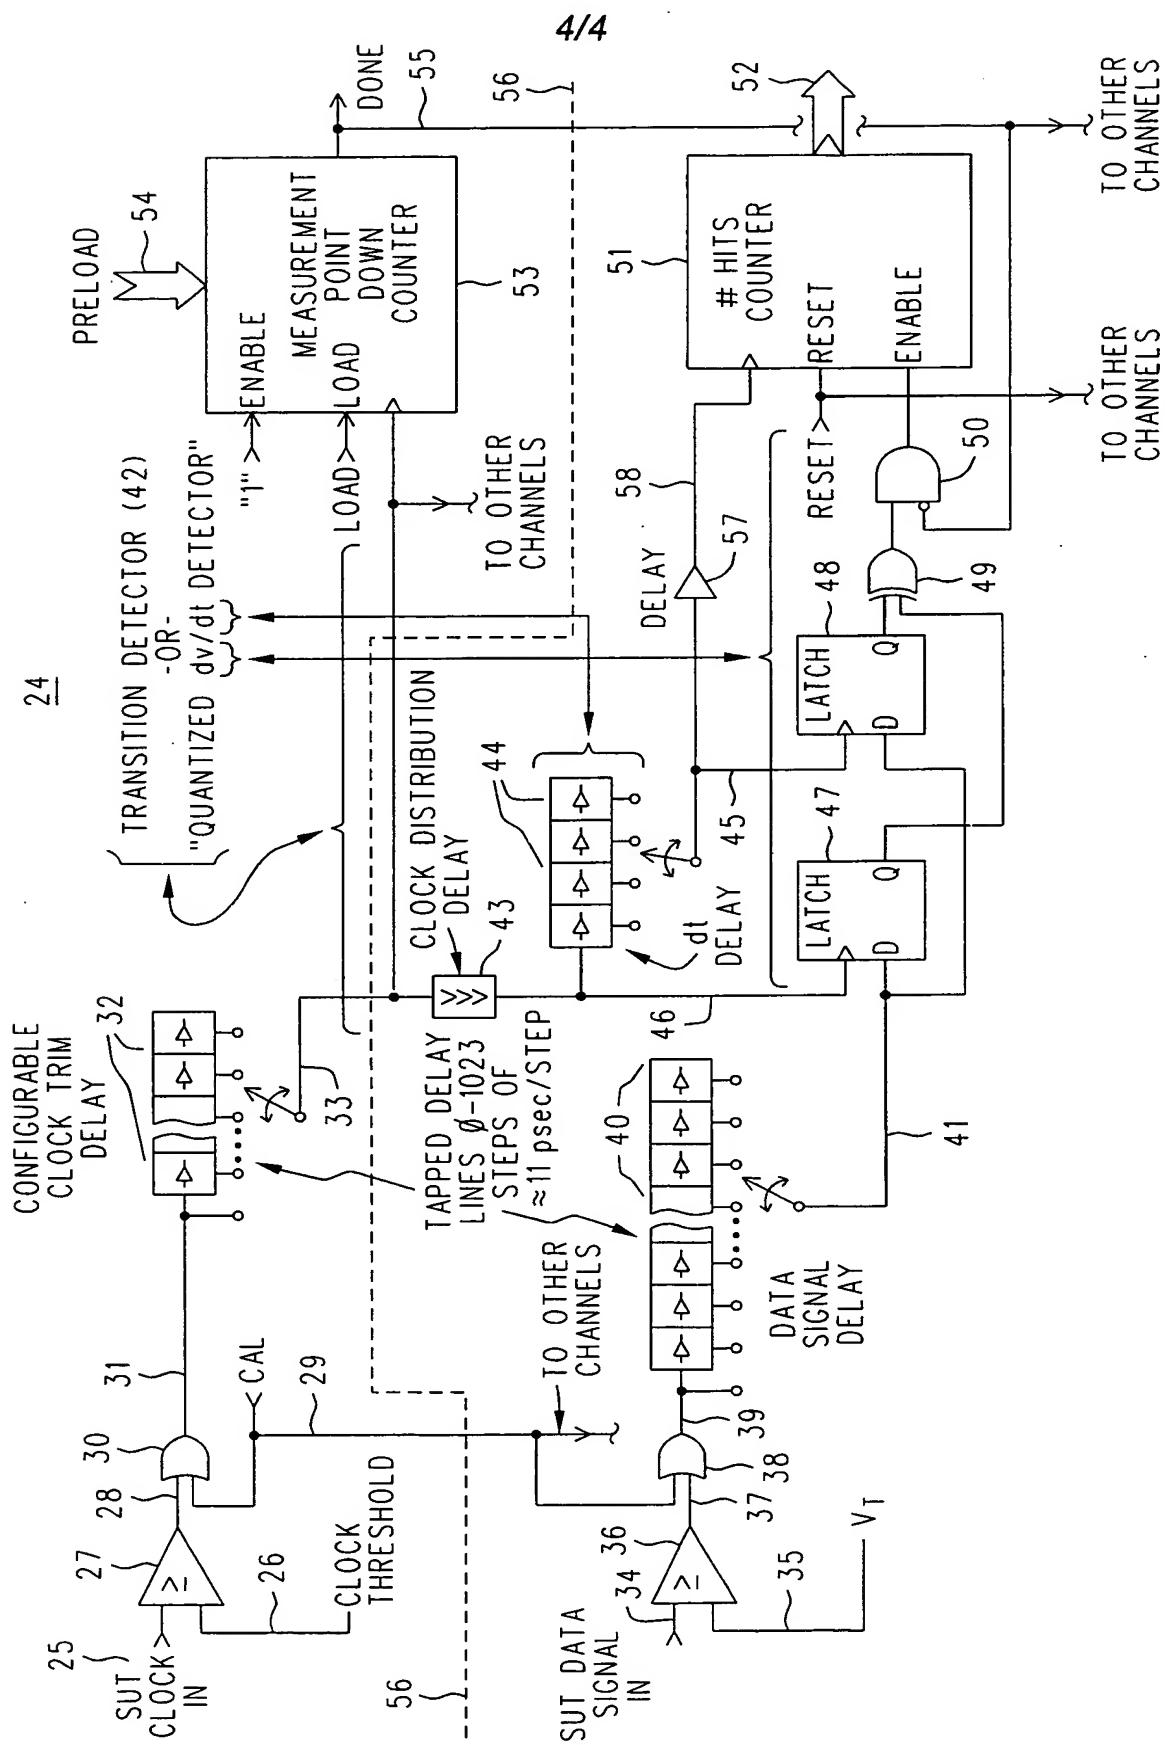


FIG. 4